

## WORST CASE OF RELATIVE DISTURBANCE GAIN ARRAY FOR UNCERTAIN DISTILLATION SYSTEM

Rudy Agustriyanto<sup>\*)</sup> and Jie Zhang

1. Chemical Engineering, Surabaya University, Surabaya 60292, Indonesia
2. School of Chemical Engineering and Advanced Materials, Newcastle University, Newcastle Upon Tyne, NE1 7RU, UK

<sup>\*)</sup>E-mail: us6193@yahoo.com

---

### Abstract

This article discusses the constrained nonlinear optimization formulation for calculating the worst case of lower and upper bounds of relative disturbance gain array (RDGA) for uncertain process models. The proposed approach seeks the minimum and maximum values of the relative disturbance gains subject to the constraints in which the process and disturbance gains are within their uncertainty ranges. RDGA ranges are useful for control structure determination and the related robustness, as they provide information regarding the sensitivity to gain uncertainties. The proposed method is demonstrated by ternary distillation column case study. Closed loop simulation results support the analysis based on the proposed method. It is shown that for a particular degree of uncertainties, the range of process gain determinant should not include zero to ensure the successfulness of the calculation. For the distillation system being studied, the maximum allowable  $\alpha$  is 0.339 to avoid the singularity of matrix  $K$ .

### Abstrak

**Kondisi Terburuk Harga *Relative Disturbance Gain Array* untuk Sistem Distilasi Tak Pasti.** Artikel ini mempresentasikan formulasi optimisasi nonlinear terbatas untuk menghitung kondisi terburuk batas bawah dan batas atas harga *relative disturbance gain array* (RDGA) untuk suatu model proses yang mengandung ketidakpastian. Pendekatan yang diusulkan adalah untuk mencari harga *relative disturbance gain* minimum dan maksimum sesuai batasan kisaran ketidakpastian yang terdapat baik pada *gain* proses maupun *gain* gangguan. Kisaran RDGA berguna untuk penentuan struktur pengendali dan ketegarannya (*robustness*) karena menyediakan informasi terkait sensitivitasnya terhadap ketidakpastian harga *gain*. Metode yang diusulkan kemudian diaplikasikan pada studi kasus kolom distilasi. Hasil simulasi lintas tertutup mendukung analisis yang didasarkan pada metode yang diusulkan. Pada kasus yang dipelajari, ditunjukkan bahwa untuk suatu derajat ketidakpastian tertentu, kisaran determinan *gain* tidak boleh mencakup titik nol untuk menjamin keberhasilan perhitungan. Untuk kasus sistem distilasi yang dipelajari, harga maksimum ketidakpastian,  $\alpha$  adalah 0.339 untuk menghindari singularitas matrix  $K$  (*gain*).

*Keywords: distillation control, relative disturbance gain array, relative gain array*

---

### 1. Introduction

With a given set of controlled and manipulated variables, controllability analysis can be performed to the system for selecting control configuration [1]. A system is said to be controllable if the controlled variables can be maintained at their set points in steady states, in spite of disturbances entering the systems. For a square system, a system is controllable if the determinant of the gain matrix is non-zero.

Decentralized (multi-loop) control relies heavily on steady state tools such as the relative gain array (RGA)

[2], Niederlinski Index (NI) [3], relative disturbance gain (RDG) and relative normalized gain array (RNGA) [4-5]. RGA has found widespread acceptance both in academia and industry since its introduction over 40 years ago, particularly after the improvement on closed loop stability considerations using NI as a stability criteria. The RGA–NI rule for decentralized control are summarized as follows [6]: a) The original RGA offers an interaction rule by its size (the paired RGA elements should be the closest to 1 and large RGA elements should be avoided), b) The NI provides a necessary stability condition by its sign (avoid pairings with negative NI), c) The signs of the RGA elements lead to

the integrity rules (all the paired RGA elements must be positive), d) The sensitivity of the RGA elements to gain uncertainties presents the robustness rule.

The popularity of RGA is mainly because of its simplicity and confirmed reliability in many case studies. However, RGA has been known to have some deficiencies, as it does not consider dynamics and disturbances. Based on the process and disturbance transfer function models, Stanley *et al.* [4] proposed RDG for analyzing the disturbance rejection capability in multi-loop control. RDG overcomes one of the limitations of RGA by allowing disturbances to be included in operability analysis. Chang and Yu extended this concept by introducing relative disturbance gain array (RDGA) and generalized relative disturbance gain array (GRDG) [7].

Recently, Chen and Seborg [8] presented an analytical expression for RGA uncertainty bounds. Two types of model uncertainty were considered: worst case bounds, where all elements of the steady state process gain matrix are allowed to change simultaneously within their bounds, and statistical uncertainty bounds. A different method by using the structured singular value ( $\mu$ ) analysis framework was introduced for the calculation of the magnitude of the worst-case relative gain [9].

Agustriyanto and Zhang [10] reported a method for calculating uncertainty bounds for relative disturbance gain via optimization for the calculation of RDGA range under model uncertainties. The model uncertainty type considered is worst-case bounds. The lower and upper bounds of an RDGA element are calculated as two constrained optimization problems. The method seeks the minimum (for the lower bound) or maximum (for the upper bound) of an RDGA element subject to the constraints that allowable model parameters are within their uncertainty bounds. RDGA ranges are shown to be important for control pairing analysis. In this paper, closed loop simulation was then performed to evaluate the RDGA analysis.

## 2. Methods

The RDGA matrix of a non-singular square matrix  $K$  and a vector disturbance  $K_d$  can be determined as follows [7]:

$$RDGA = \left[ K^{-1} \text{diag}(K_d) \right]^{-1} \left[ \text{diag}(K^{-1} K_d) \right] \quad (1)$$

where  $\text{diag}(\cdot)$  transforms a vector  $(\cdot)$  into a diagonal matrix with each element put on the corresponding diagonal position, that is, the  $i$ th element of a vector  $(\cdot)$  is put on the  $i$ th entry of a matrix.

Each element of RDGA matrix is related to the corresponding element of RGA matrix through the

following relationship:

$$\beta_{ij} = \lambda_{ij} + \sum_{\substack{k=1 \\ k \neq i}}^n \frac{K_{ij} \tilde{K}_{jk} K_{dk}}{K_{di}} \quad (2)$$

where  $\beta_{ij}$  = element of RDGA matrix

$\lambda_{ij}$  is the  $ij$  th element of the RGA

$\tilde{K}_{ik}$  is the element on the  $i$ th row and  $k$ th column of  $K^{-1}$

The following equation is the relation between  $ij$ th element of RGA and steady state gains matrix [11]:

$$\lambda_{ij} = (-1)^{i+j} \frac{K_{ij} \det(K^{ij})}{\det(K)} \quad (3)$$

In Eq. (3),  $K^{ij}$  is the submatrix that remains after the  $i$ th row and  $j$ th column of  $K$  are deleted.

It is obvious that  $\beta_{ij}$  is a function of  $K$  and  $K_d$ , that is

$$\beta_{ij} = f(K, K_d) \quad (4)$$

Assuming that the uncertainty bounds for all steady state process and disturbance gains  $K_{ij}$  and  $K_{di}$  are given, then there will be  $2(n2+n)$  constraints for all those gains which can be formulated as follows:

$$AX \leq b \quad (5)$$

where  $X$  is a vector of size  $(n2+n) \times 1$  containing all elements of  $K$  and  $K_d$  as its elements:

$X = [K_{11} \dots K_{nn} K_{d1} \dots K_{dn}]^T$ ,  $b$  is a vector of size  $(2(n2+n)) \times 1$  containing the lower and upper bound values of the corresponding elements of  $X$ , and  $A$  is an appropriate matrix of size  $(2(n2+n)) \times (n2+n)$  satisfying the inequalities in Eq.(5).

Therefore, the lower bound and the upper bound of  $\beta_{ij}$  can be formulated as the following respectively:

Lower bound:

$$\min_X \beta_{ij} = f(X) \quad (6)$$

Upper bound:

$$\max_X \beta_{ij} = f(X) \quad (7)$$

both subject to the constraints in Eq.(4).

Note that  $\beta_{ij}$  cannot be determined if the value of  $\det(K) = 0$ . Furthermore, when  $\det(K) = 0$ , the process will be uncontrollable in that some controlled variables will be dependent to each other and will not be able to follow independent set point changes. Therefore, in order to use the above method and also to ensure the process is controllable, the range of  $\det(K)$  should not include 0. The range of  $\det(K)$  can be considered as a function of

all the individual elements of the gain matrix:

$$\det(K) = g(X) \quad (8)$$

The range of  $\det(K)$  can be calculated by using the same optimization method:

Lower bound:

$$\min_X \det(K) = g(X) \quad (9)$$

Upper bound:

$$\max_X \det(K) = g(X) \quad (10)$$

both subject to the same constraints in Eq.(5).

The RDGA matrix in conjunction with the structure selection matrix is used to determine the so-called GRDG, which is useful for control structure selection. A structure selection matrix is an  $n \times n$  matrix where the  $ij$ th entry is set equal to 1 if the element is chosen for controller pairing or equal to zero if the element is ignored. The value of GRDG vector element is simply the row wise summation of RDGA with the corresponding structure selection matrix.

There are various numerical methods that can be used to solve this constrained optimization problem, such as grid search, random jumping method, the generalized reduced gradient algorithm, etc [12-13]. By using grid search optimization, RDGA in Eq.(1) can be evaluated at all combination points that are specified between the uncertainty bounds of  $K$  and  $K_d$  in nested loop and hence RDGA ranges are determined by sorting out the minimum and maximum values of each element from all the computed RDGAs. This method requires huge number of RDGA calculation, which cannot be avoided. By dividing each element of each gain into only 2 equal segments (3 nodes) then for  $3 \times 3$  size of  $K$  matrix and  $3 \times 1$   $K_d$  matrix, it will require  $3^{(9+3)} = 531,441$  calculations. This method generally is not preferred since the number of segments/nodes must be increased for more precise calculation. Moreover, most plant wide control problem involves many control, manipulating and disturbance variables, which contribute to the rapid increase of the number of calculation.

In random jumping method, random values of each element of  $K$  and  $K_d$  between their bounds are generated and the RDGA is evaluated at this point. Calculation is performed for large number of random points of  $K$  and  $K_d$  and the RDGA ranges are picked from the total results. This method is simple and fairly acceptable for this purpose. Other advance optimization techniques may require gradient of the function for generating new point for iteration. However, the availability of the optimizer such as Matlab Optimization Toolbox (e.g. *fmincon*) makes computation become faster and able to provide accurate results without bothering about derivatives of the function, which is often difficult to obtain. The formulated problem can be readily solved in

this Matlab environment. A satisfactory result can be obtained by initiating the optimization from different starting point within the bounds if the objective function exhibits many local optima.

### 3. Results and Discussion

In this example we consider the two distillation column system for separating benzene, toluene and m-xylene [14]. The process transfer function matrix,  $G(s)$ , and the disturbance transfer function matrix,  $G_d(s)$ , of the Ding and Luyben (DL) column are as follows:

$$G(s) = \begin{bmatrix} \frac{-11.5e^{-s}}{(23s+1)(5s+1)} & 0 & 0 \\ \frac{3.75e^{-2s}}{(14s+1)(3s+1)^2} & \frac{1.6e^{-1.3s}}{(13s+1)(3s+1)} & \frac{-1.2e^{-10.5s}}{(15.5s+1)(3s+1)} \\ \frac{20.6e^{-1.9s}}{(23s+1)(18s+1)} & \frac{-7.5e^{-2.3s}}{(37.3s+1)(2s+1)} & \frac{23.1e^{-s}}{(42s+1)(2s+1)} \end{bmatrix} \quad (11)$$

$$G_d(s) = \begin{bmatrix} \frac{-1.95e^{-5s}}{(12s+1)^2} \\ \frac{1.52e^{-6s}}{(12s+1)^2(5s+1)} \\ \frac{-4.45e^{-7s}}{(40s+1)(10s+1)^2} \end{bmatrix} \quad (12)$$

The process outputs are:

$y_1$  = composition of benzene from top of column 1

$y_2$  = composition of toluene from top of column 2

$y_3$  = composition of m-xylene from bottom of column 2.

The manipulated variables are:

$u_1$  = heat transfer to reboiler 1

$u_2$  = reflux rate at column 2

$u_3$  = heat transfer to reboiler 2

The disturbance variable is:

$d$  = feed composition type 3 (30%, 40%, 30%) or 4 (20%, 60%, 20%).

The nominal value of RDGA calculated using Eq.(1) is:

$$RDGA = \begin{bmatrix} 1 & 0 & 0 \\ 0.42 & 0.41 & 0.17 \\ -0.79 & 0.66 & 1.13 \end{bmatrix} \quad (13)$$

Assuming now that the uncertainty bounds for all processes and disturbance steady state gain  $K_{ij}$  and  $K_{di}$  are given by

$$|\Delta K_{ij}| \leq \alpha |\hat{K}_{ij}| \quad (14)$$

$$|\Delta K_{di}| \leq \alpha |\hat{K}_{di}| \quad (15)$$

Similar to what have been done for the nominal case [7], GRDG analysis is performed for the three cases of uncertain models. The results are compared to the nominal value analysis. The controller structures are limited to be of diagonal, block diagonal (bd), and full multivariable structures.

The uncertainty ranges for RDGA calculated by random jumping method are shown below in Eq.(16–18) for the case of  $\alpha = 0.01, 0.1$  and  $0.25$  respectively.

$$RDGA_1 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.40 \leq \beta_{21} \leq 0.43 & 0.38 \leq \beta_{22} \leq 0.44 & 0.16 \leq \beta_{23} \leq 0.19 \\ -0.81 \leq \beta_{31} \leq -0.76 & 0.60 \leq \beta_{32} \leq 0.72 & 1.05 \leq \beta_{33} \leq 1.21 \end{bmatrix} \quad (16)$$

$$RDGA_2 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.28 \leq \beta_{21} \leq 0.62 & 0.06 \leq \beta_{22} \leq 0.68 & 0.02 \leq \beta_{23} \leq 0.37 \\ -1.15 \leq \beta_{31} \leq -0.54 & 0.08 \leq \beta_{32} \leq 1.52 & 0.19 \leq \beta_{33} \leq 2.01 \end{bmatrix} \quad (17)$$

$$RDGA_3 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.16 \leq \beta_{21} \leq 1.10 & -1.16 \leq \beta_{22} \leq 1.07 & -0.32 \leq \beta_{23} \leq 1.32 \\ -1.95 \leq \beta_{31} \leq -0.30 & -1.71 \leq \beta_{32} \leq 4.02 & -2.23 \leq \beta_{33} \leq 4.11 \end{bmatrix} \quad (18)$$

As a comparison, Eq. (19-21) below are the results computed by using Matlab Optimization Toolbox. It is shown that wider ranges can be obtained compared to previous results using random jumping method. Therefore, the GRDG analysis for uncertain system presented in this paper will be based on the RDGA results computed by Matlab Optimization Toolbox due to its accuracy

$$RDGA_1 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.40 \leq \beta_{21} \leq 0.44 & 0.37 \leq \beta_{22} \leq 0.45 & 0.15 \leq \beta_{23} \leq 0.20 \\ -0.82 \leq \beta_{31} \leq -0.75 & 0.57 \leq \beta_{32} \leq 0.75 & 1.02 \leq \beta_{33} \leq 1.23 \end{bmatrix} \quad (19)$$

$$RDGA_2 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.28 \leq \beta_{21} \leq 0.62 & -0.11 \leq \beta_{22} \leq 0.74 & -0.02 \leq \beta_{23} \leq 0.49 \\ -1.17 \leq \beta_{31} \leq -0.53 & -0.18 \leq \beta_{32} \leq 1.77 & -0.13 \leq \beta_{33} \leq 2.26 \end{bmatrix} \quad (20)$$

$$RDGA_3 = \begin{bmatrix} 1 \leq \beta_{11} \leq 1 & 0 \leq \beta_{12} \leq 0 & 0 \leq \beta_{13} \leq 0 \\ 0.15 \leq \beta_{21} \leq 1.16 & -3.51 \leq \beta_{22} \leq 1.93 & -1.08 \leq \beta_{23} \leq 3.35 \\ -2.18 \leq \beta_{31} \leq -0.28 & -7.98 \leq \beta_{32} \leq 8.60 & -7.13 \leq \beta_{33} \leq 11.16 \end{bmatrix} \quad (21)$$

GRDG analysis for the nominal model (Table 1) shows that the block diagonal controller bd [(1,3),2] offers the best disturbance rejection capability [7]. Small values of GRDG elements are preferable since they reflect the ratio of net load effect over the open loop load effect. The GRDG values for the three cases of model uncertainties are presented in Table 2.

For  $\alpha = 0.01$ , it is obvious from Table 2 that the block diagonal controller bd [(1,3),2] will be recommended. However, as the value of  $\alpha$  increased to 0.1 and 0.25, it can be predicted that bd [(1,3),2] will be no longer the best choice. The performance of this control structure may not be as good as the diagonal control structure.

**Table 1. GRDG for the Nominal Model of the DL Column**

Control Structure	GRDG		
Diagonal	[1.00	0.41	1.13] <sup>T</sup>
bd [(1,2),3]	[1.00	0.83	1.13] <sup>T</sup>
bd [(1,3),2]	[1.00	0.41	0.34] <sup>T</sup>
bd [(2,3),1]	[1.00	0.58	1.79] <sup>T</sup>
Full	[1.00	1.00	1.00] <sup>T</sup>

**Table 2. GRDG for Uncertainty Models of the DL Column**

Control structure	$\alpha = 0.01$	$\alpha = 0.1$	$\alpha = 0.25$
Diagonal	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.3695 \leq \delta_2 \leq 0.4488 \\ 1.0215 \leq \delta_3 \leq 1.2324 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -0.1101 \leq \delta_2 \leq 0.7390 \\ -0.1254 \leq \delta_3 \leq 2.2611 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -3.5142 \leq \delta_2 \leq 1.9336 \\ -7.1287 \leq \delta_3 \leq 11.1648 \end{bmatrix}$
bd [(1,2),3]	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.7714 \leq \delta_2 \leq 0.8842 \\ 1.0215 \leq \delta_3 \leq 1.2324 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.1699 \leq \delta_2 \leq 1.3639 \\ -0.1254 \leq \delta_3 \leq 2.2611 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -3.3636 \leq \delta_2 \leq 3.0956 \\ -7.1287 \leq \delta_3 \leq 11.1648 \end{bmatrix}$
bd [(1,3),2]	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.3695 \leq \delta_2 \leq 0.4488 \\ 0.2045 \leq \delta_3 \leq 0.4782 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -0.1101 \leq \delta_2 \leq 0.7390 \\ -1.2980 \leq \delta_3 \leq 1.7356 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -3.5142 \leq \delta_2 \leq 1.9336 \\ -9.3091 \leq \delta_3 \leq 10.8822 \end{bmatrix}$
bd [(2,3),1]	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.5188 \leq \delta_2 \leq 0.6439 \\ 1.5899 \leq \delta_3 \leq 1.9803 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -0.1292 \leq \delta_2 \leq 1.2242 \\ -0.3017 \leq \delta_3 \leq 4.0287 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -4.5984 \leq \delta_2 \leq 5.2858 \\ -15.1130 \leq \delta_3 \leq 19.7644 \end{bmatrix}$
Full	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.9207 \leq \delta_2 \leq 1.0793 \\ 0.7729 \leq \delta_3 \leq 1.2261 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ 0.1508 \leq \delta_2 \leq 1.8491 \\ -1.4743 \leq \delta_3 \leq 3.5032 \end{bmatrix}$	$\begin{bmatrix} 1 \leq \delta_1 \leq 1 \\ -4.4478 \leq \delta_2 \leq 6.4478 \\ -17.2934 \leq \delta_3 \leq 19.4818 \end{bmatrix}$

Figure 1 shows that the maximum allowable  $\alpha$  for this system is 0.339 to avoid singularity of matrix  $K$ . Closed loop simulation was then performed to evaluate the control performance. PI controllers were used. For tuning purpose, the system is disturbed by the sequence of step disturbance as shown in Figure 2 and the following set-point changes:  $y_1$  set-point was changed from 0 to 1 at  $t = 450$  min;  $y_2$  set-point was changed from 0 to -1 at  $t = 550$  min;  $y_3$  set-point was changed from 0 to 1 at  $t = 650$  min.

The output values are recorded for 1000 min simulation time with 1 min sampling time. Table 3 shows the controller parameters obtained via optimization for both disturbance rejection and set point tracking during the specified time by minimizing the sum squared of error (SSE).

Simulations were then performed for the arbitrarily altered process and disturbance gains (which reflect model uncertainties) as follows:

$$\bar{G} = \begin{bmatrix} G_{11}(1-\alpha) & G_{12}(1+\alpha) & G_{13}(1-\alpha) \\ G_{21}(1+\alpha) & G_{22}(1-\alpha) & G_{23}(1+\alpha) \\ G_{31}(1-\alpha) & G_{32}(1+\alpha) & G_{33}(1-\alpha) \end{bmatrix} \quad (22)$$

$$\bar{G}_d = \begin{bmatrix} G_{d1}(1-\alpha) \\ G_{d2}(1+\alpha) \\ G_{d3}(1-\alpha) \end{bmatrix} \quad (23)$$


The profile of the considered disturbance in simulation is similar to that used for tuning purpose (Figure 2) but with larger magnitude:  $\Delta d = +5$  at  $t = 50$  min;  $\Delta d = +5$  at  $t = 150$  min;  $\Delta d = -15$  at  $t = 250$  min;  $\Delta d = +5$  at  $t = 350$  min.

Figure 3 shows the results for three different values of  $\alpha$  ranging from 0 to 0.25. It is shown that closed loop performance deteriorates as the level of model uncertainties is increased. For  $\alpha = 0.339$ , as shown in Figure 4, the control structure  $bd[(1,3),2]$  with controller parameters obtained based on the nominal model obviously fails to achieve the required control objectives.

GRDG analysis for uncertain models indicates that for increased values of  $\alpha$  (0.1 and 0.25) control structure  $bd[(1,3),2]$  may not be the best choice compared to the diagonal control structure. In order to verify the above analysis, closed loop performance was also investigated

**Table 3. Controller Parameters for the Control Structure  $bd[(1,3),2]$**

Controller	$K_c$	$T_i$
$G_{c,11}$	-1.14	36.55
$G_{c,31}$	0.01	0.29
$G_{c,13}$	-0.09	2.55
$G_{c,33}$	1.19	15.42
$G_{c,22}$	1.18	9.49

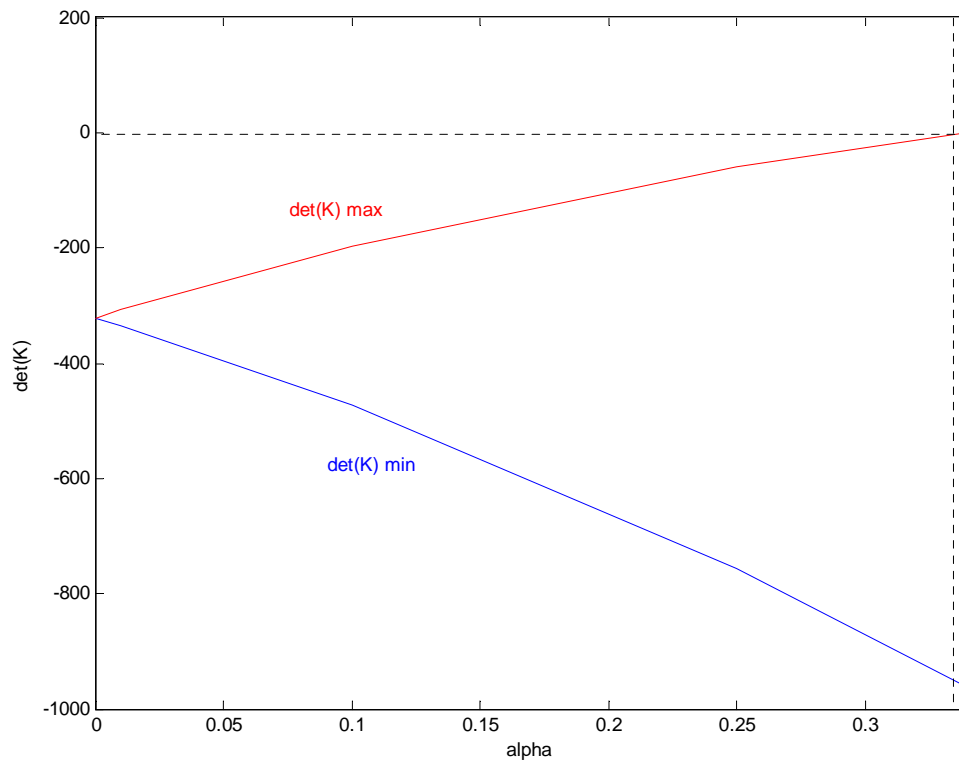

**Figure 1. Range of  $\det(K)$  vs  $\alpha$**

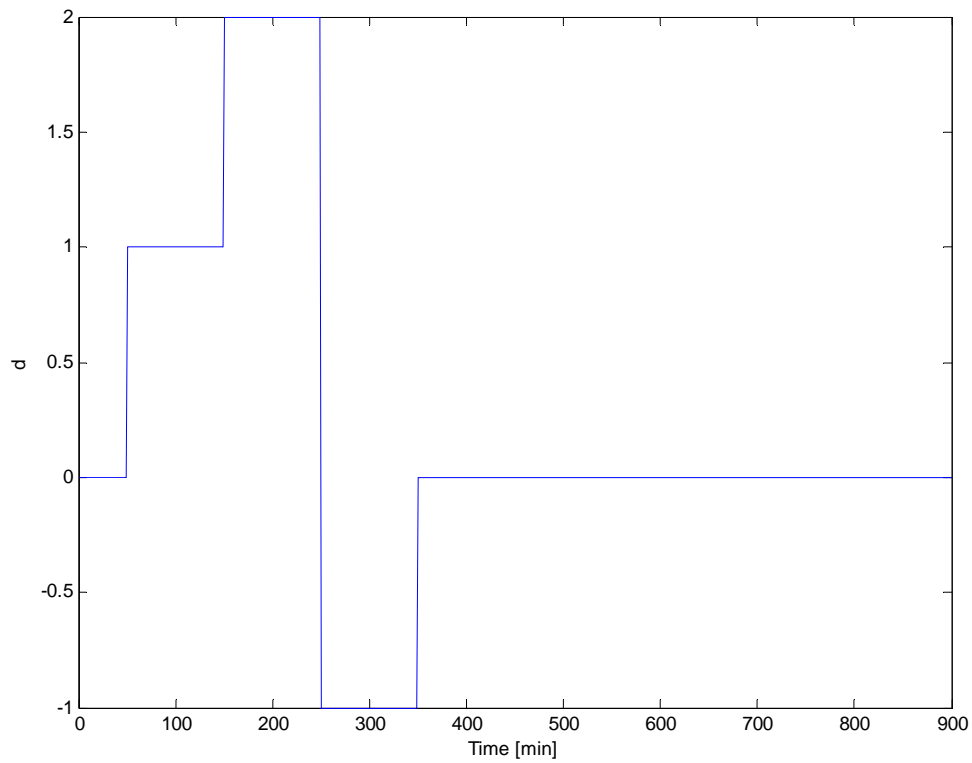


Figure 2. Profile of Disturbance for Controller Tuning

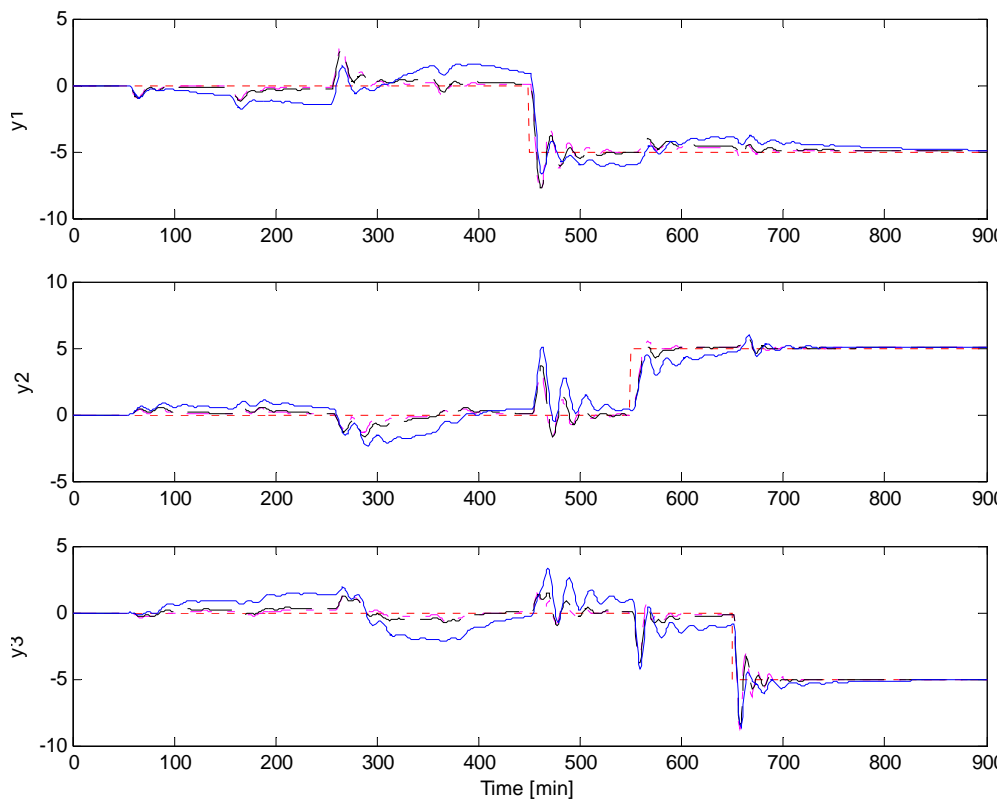


Figure 3. Simulation Results for Example 2,  $bd[(1,3),2]$ , ( $y$  setpoint, .....  $y$  for  $\alpha = 0$ , ----  $y$  for  $\alpha = 0.1$ , —  $y$  for  $\alpha = 0.25$ )

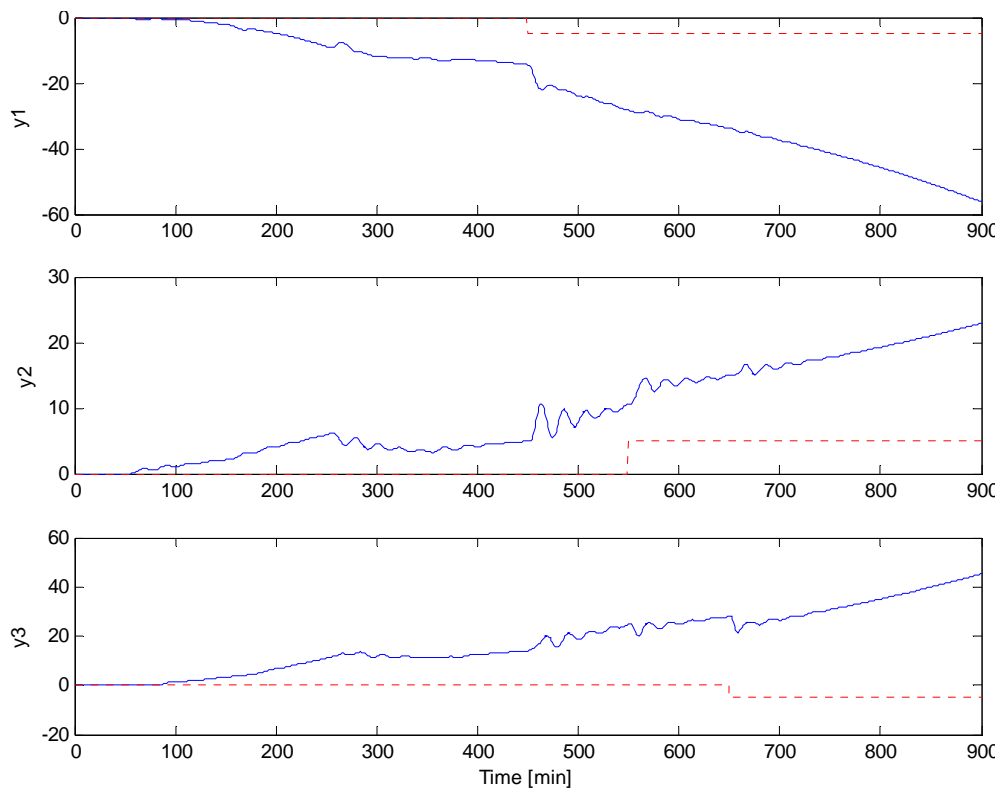


Figure 4. Simulation Results for Example 2,  $bd[(1,3),2]$ ,  $\alpha = 0.339$ , (.....)  $y$  setpoint, —  $y$  for  $\alpha = 0.339$

for the diagonal control structure. Table 4 shows the controller parameters obtained via optimization for the diagonal control structure ( $y_1 - u_1, y_2 - u_2, y_3 - u_3$ ).

Figure 5 shows the simulation results for three different values of  $\alpha$  ( $\alpha = 0, 0.1$  and  $0.25$ ). It can be seen that the diagonal control structure with nominal controller settings gives better performance than  $bd[(1,3),2]$  when  $\alpha = 0.25$ . The SSE values from the two different control structures are presented in Table 5. It is shown that for small values of  $\alpha$  ( $\alpha = 0$  and  $0.01$ ), the control performance of  $bd[(1,3),2]$  is better than that of the diagonal structure, i.e. with lower SSE values. The results support the above GRDG analysis that as the value of  $\alpha$  is increased to  $0.1$  or  $0.25$  (Table 4), it becomes harder to see that  $bd[(1,3),2]$  is the best choice or not.

The closed loop performance in term of SSE as presented in Table 5 were obtained based on controller setting for the nominal process (i.e.  $\alpha = 0$ ). However, for uncertain systems, it is not necessary to find controller settings for the nominal model. Table 6 provides alternative controller settings for both  $bd[(1,3),2]$  and diagonal structures obtained based on the altered gains in Eq. (22) and Eq. (23) for different values of  $\alpha$ . Optimization tuning method was used to obtain the best performance (minimum SSE) for each case. Each set of controller setting was then tested on other values

Table 4. Controller Parameters for the Diagonal Control Structure

Controller	$K_c$	$T_i$
$G_{c,11}$	-1.15	33.32
$G_{c,22}$	1.08	8.53
$G_{c,33}$	1.17	13.29

Table 5. SSE Comparison between  $bd[(1,3),2]$  and the Diagonal Control Structure

$\alpha$	$bd[(1,3),2]$	Diagonal
0	835.75	937.80
0.01	842.69	939.52
0.1	977.78	996.70
0.25	2238.6	1601.10
0.339	$1.8131 \times 10^6$	3314.60

of  $\alpha$  and their closed loop performances in term of SSE are compared in Table 7. The following conditions were used for both tuning and simulation purposes: 1) A series of step disturbance ( $\Delta d$ ) = +1, +1, -3 and +1 at  $t = 50, 150, 250$  and  $350$  min respectively, 2)  $y_1$  set-point was changed from 0 to 1 at  $t = 450$  min, 3)  $y_2$  set-point was changed from 0 to -1 at  $t = 550$  min, 4)  $y_3$  set-point was changed from 0 to 1 at  $t = 650$  min, 5) simulation time = 1000 min.

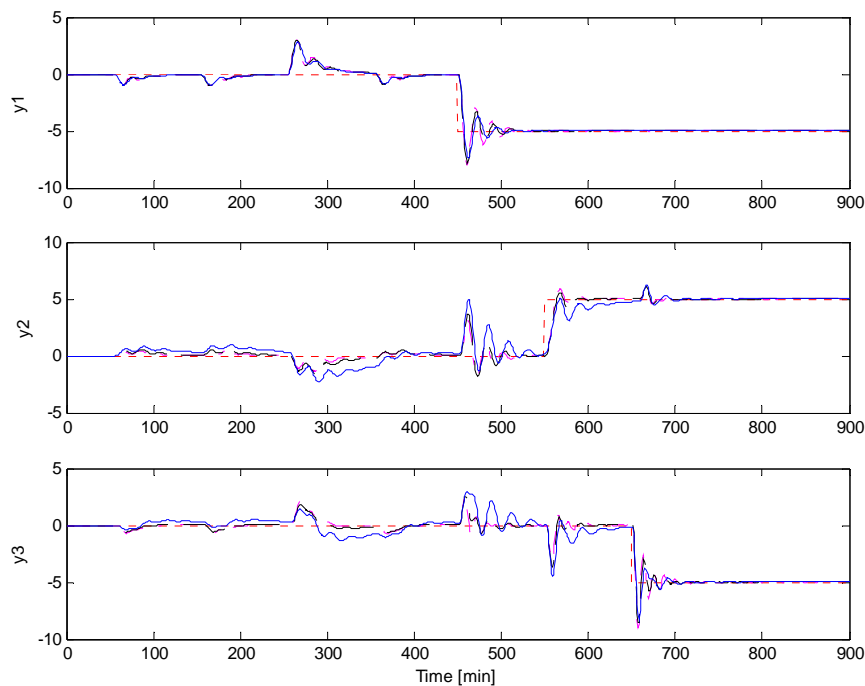


Figure 5. Simulation Results for Example 2, Diagonal,  $\alpha = 0, 0.1$  and  $0.25$ , ( .....y setpoint, -----y for  $\alpha = 0$ , y for  $\alpha = 0.1$ , —y for  $\alpha = 0.25$ )

Table 6. Controller Parameters based on Different Values of  $\alpha$

$\alpha$	Control Structure	Controller	$K_c$	$T_i$
0.01	bd[(1,3),2]	$G_{c,11}$	-1.14	32.01
		$G_{c,31}$	0.10	1.81
		$G_{c,13}$	-0.23	6.24
		$G_{c,33}$	1.26	15.17
		$G_{c,22}$	1.19	8.76
	diagonal	$G_{c,11}$	-1.16	33.65
0.1	bd[(1,3),2]	$G_{c,22}$	1.07	8.31
		$G_{c,33}$	1.18	13.43
		$G_{c,11}$	-1.20	41.09
		$G_{c,31}$	$2.9896 \times 10^{-4}$	0.01
		$G_{c,13}$	-0.14	4.37
	diagonal	$G_{c,33}$	1.38	15.49
		$G_{c,22}$	1.11	7.55
		$G_{c,11}$	-1.23	37.13
		$G_{c,22}$	0.96	6.62
		$G_{c,33}$	1.30	14.24
0.25	bd[(1,3),2]	$G_{c,11}$	-1.14	33.35
		$G_{c,31}$	0.0011	1
		$G_{c,13}$	-0.19	21
		$G_{c,33}$	1.62	10.57
		$G_{c,22}$	0.82	4.46
	Diagonal	$G_{c,11}$	-1.25	37.42
		$G_{c,22}$	0.73	4.25
		$G_{c,33}$	1.49	10.07

Table 7. SSE Comparison for bd[(1,3),2] and Diagonal Control Structures for Different Controller Settings

$\alpha$ as controller setting basis	$\alpha$ for closed loop performance test	bd[(1,3),2] SSE	diagonal SSE
0.01	0	32.85	37.41
	0.01	33.09	37.46
	0.1	38.05	39.50
	0.25	116.39	60.53
	0.339	12327	134.98
0.1	0	34.81	38.22
	0.01	34.79	38.12
	0.1	36.81	38.94
	0.25	73.24	56.75
	0.339	474.71	126.30
0.25	0	82.04	72.74
	0.01	74.20	66.34
	0.1	45.87	45.04
	0.25	50.90	51.53
	0.339	94.82	94.66

Closed loop performance comparison presented in Table 7 can be summarized as the following: 1) For controller parameters obtained based on the altered gains at  $\alpha = 0.01$ , similar closed loop performance as that using nominal model based settings were obtained. On these settings, bd[(1,3),2] gives better performance (smaller SSE values) when tested on low  $\alpha$  values (0, 0.01 and

0.1) while the diagonal control structure gives better performance on other  $\alpha$  values; 2) Controller parameters based on  $\alpha = 0.1$  also show that  $bd[(1,3),2]$  was better when the system is tested on  $\alpha = 0, 0.01$  and  $0.1$  for the specified altered process; 3) By using controller parameters obtained based on  $\alpha = 0.25$ , the closed loop performance shows that the diagonal control structure was better for all cases; 4) Both  $bd[(1,3),2]$  and diagonal control structures give relatively similar SSE values when tested on  $\alpha = 0.1$ . This evidence support the GRDG prediction that as the value of  $\alpha$  increased to  $0.1$  and  $0.25$ , it becomes harder to see that  $bd[(1,3),2]$  is the best choice or not.

#### 4. Conclusions

This paper discusses an alternative method for determining worst case lower and upper bounds RDGA ranges for uncertain process models. Constrained optimization is used to find the uncertain RDGA ranges. The proposed method is applied to the ternary distillation column. It is shown that the proposed method is easy to use and gives accurate results. Closed loop simulation results confirm the analysis based on the proposed method.

#### Acknowledgement

This work was supported by Technological and professional Skills Development Sector Project (TPSDP)–ADB Loan No. 1792–INO. This support is gratefully acknowledged.

#### References

- [1] S. Skogestad, *Comput. Chem. Eng.* 28 (2004) 219.
- [2] E. Bristol, *IEEE Trans. Autom. Control* 11/1 (1996) 133.
- [3] A. Niederlinski, *Automatica* 7/6 (1971) 691.
- [4] G. Stanley, M. Marino-Galarraga, T.J. McAvoy, *Ind. Eng. Chem. Process Des. Dev.* 24/4 (1985) 1181.
- [5] M.J. He, W.J. Cai, W. Ni, L.H. Xie, *J. Process Control* 19 (2009) 1036.
- [6] Z.X. Zhu, *Ind. Eng. Chem. Res.* 35/11 (1996) 4091.
- [7] J.W. Chang, C.C. Yu, *AIChE J.* 38/4 (1992) 521.
- [8] D. Chen, D.E. Seborg, *AIChE J.* 48/2 (2002) 302.
- [9] V. Kariwala, S. Skogestad, J.F. Forbes, *Ind. Eng. Chem. Res.* 45/5 (2006) 1751.
- [10] R. Agustriyanto, J. Zhang, *Proc. of the 2007 American Control Conference*, New York, USA, 2007, p.5360.
- [11] P. Grosdidier, M. Morari, B.R. Holt, *Ind. Eng. Chem. Fundam.* 24/2 (1985) 221.
- [12] S.S. Rao, *Engineering Optimization–Theory & Practice*, 4<sup>th</sup> ed., John Wiley & Sons, Inc, 2009, p.840.
- [13] T.F. Edgar, D.M. Himmelblau, L.S. Lasdon, *Optimization of Chemical Processes*, McGraw-Hill, 2001, p.672.
- [14] S.S. Ding, W. Luyben, *Ind. Eng. Chem. Res.* 29/7 (1990) 1240.