

DEVELOPMENT OF A POTENTIOMETRIC SENSOR SENSITIVE TO POLYSORBATE 20

Maria Mironyak

*Department of Analytical Chemistry and Chemical Technology of Food Additives and Cosmetics
Ukrainian State University of Chemical Technology
8 Gagarina ave., Dnipro, Ukraine, 49005
mari_mir@i.ua*

Olena Volnyanska

*Department of Analytical Chemistry and Chemical Technology of Food Additives and Cosmetics
Ukrainian State University of Chemical Technology
8 Gagarina ave., Dnipro, Ukraine, 49005
olena.volnianskia@ukr.net*

Oksana Labyak

*Department of Analytical Chemistry and Chemical Technology of Food Additives and Cosmetics
Ukrainian State University of Chemical Technology
8 Gagarina ave., Dnipro, Ukraine, 49005
oksanalabyak777@gmail.com*

Vadym Kovalenko

*Department of Analytical Chemistry and Chemical Technology of Food Additives and Cosmetics
Ukrainian State University of Chemical Technology
8 Gagarina ave., Dnipro, Ukraine, 49005
Competence center "Ecological technologies and systems"
Vyatka State University
36 Moskovskaya str., Kirov, Russian Federation, 610000
vadimchem@gmail.com*

Valerii Kotok

*Department of Processes, Apparatus and General Chemical Technology
Ukrainian State University of Chemical Technology
8 Gagarina ave., Dnipro, Ukraine, 49005
Competence center "Ecological technologies and systems"
Vyatka State University
36 Moskovskaya str., Kirov, Russian Federation, 610000
valeriykotok@gmail.com*

Abstract

Polyoxyethylated sorbitans (polysorbates) are widely used in the chemical, pharmaceutical, and cosmetic industries, but only quantitative determination is used mainly for chromatographic methods. In this paper, the results of the development and testing of a potentiometric sensor sensitive to nonionic surfactant polyoxyethylene sorbitan monolaurate (polysorbate-20) are presented. An anion of the heterogeneous acid of the Keggin structure (12-molybdophosphate heteropolyacid) was used as a counterion to obtain the electrode-active substance for the potentiometric sensor membrane. Polysorbate-20 does not form cations when dissociating in water and cannot directly interact with heteropolyanion; therefore, a cationic complex of polysorbate-20 with barium ions was previously prepared (similar to the interaction of metals with crown ethers). The resulting ion associate meets the basic requirement for the electrode-active substance of plasticized film polyvinyl chloride membranes of potentiometric sensors (poor water solubility and good solubility in organic solvents). Phthalic acid derivatives (dibutyl phthalate and dioctyl phthalate) were used as solvent-plasticizers for a polyvinyl chloride membrane. To determine the optimum conditions for the functioning of a potentiometric sensor sensitive to polysorbate-20, the influence of various factors on the electrode characteristics was studied. Quantitative content of the ionic associate in the polyvinyl chloride membrane, the nature of the membrane solvent-plasticizer, pH of a series of standard polysorbate-20 solutions) on the electrode characteristics

of the plasticized membrane of the potentiometric sensor (sensitivity or slope of the electrode function, lower limit of linearity and minimum detectable concentration of polysorbate-20, which can be determined with the help of the developed potentiometric sensor) was studied. The optimal conditions for using the developed potentiometric sensor were found. The developed sensor allows for a short period of time (5–10 min) determining the quantitative content of polysorbate-20 in industrial products at the level 10^{-5} – 10^{-6} mol/l. The potentiometric sensor sensitive to polysorbate-20 can be used for the development of a potentiometric method for determining the clinical reception of polysorbate-20 in various types of industrial products.

Keywords: 12-molybdophosphate heteropolyacid, polyoxyethylene sorbitans, polysorbate, potentiometric sensor, direct potentiometry, tween.

DOI: 10.21303/2461-4262.2019.00942

1. Introduction

Polysorbates (trade name “tween”) are ethoxylated sorbitans exhibiting the properties of non-ionic surfactants. These compounds are widely used in industry as fiber softeners, defoamers, antistatic agents, emulsifiers and solubilizes [1].

Polyoxyethylene sorbitan monolaurate (Polysorbate-20) is a non-ionic surfactant with a degree of ethoxylation at 20 (**Fig. 1**). It was chosen as the object of a study.

Polysorbate-20 is used in the cosmetic industry [1–4]: to improve the dissolution of essential oils; in foam-washing compositions, which are moisturizing well, don't irritate and don't overdry the skin; in decorative cosmetics.

Currently, IR spectroscopy is used to identify ethoxylated sorbitans [5], and high-performance liquid chromatography [6–10] is used to quantify the content. According to previous studies [11–20], direct potentiometry using sensors which are sensitive to organic cations and substances is a simple, rapid and sensitive method of determination. The purpose of this study was to develop a potentiometric sensor which would allow to quickly and efficiently determine polysorbate-20 in various environmental objects and industrial products.

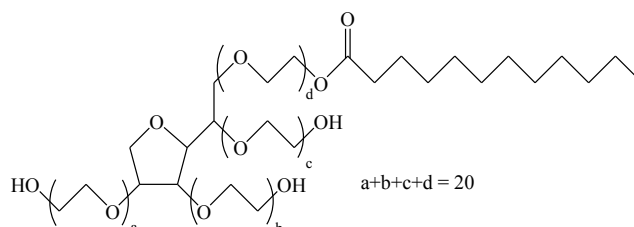


Fig. 1. Polysorbate 20 structural formula

Inasmuch as the ethoxylated sorbitans are non-ionic surfactants and don't form ions upon dissolution, a cationic complex of polysorbate-20 with barium ions was obtained in advance to obtain an associate with a 12-molybdophosphate heteropolyacid.

2. Methods, materials, and devices, used for making and testing of the potentiometric sensor for polysorbate 20 detection

2. 1. Materials used for developing and testing of the potentiometric sensor for polysorbate 20 detection

The following reagents are used in the work:

- 12-molybdophosphate acid, $H_3PMo_{12}O_{40} \times 26H_2O$ (analytically pure);
- Polysorbate-20, $C_{58}H_{114}O_{26}$ (pure grade);
- Sodium hydroxide (analytically pure);
- Chloride acid (conc.) (analytically pure);
- Barium nitrate (analytically pure).

The following reagents were used to manufacture membranes potentiometric sensors:

- PVC (polyvinyl chloride), brand C-70 (pure grade) is a membrane matrix;
- CH (cyclohexanone), (analytically pure) is a matrix solvent.

The phthalic acid esters are used as membrane solvent-plasticizers:

- dibutyl phthalate (DBF), pure grade;
- dioctyl phthalate (DOF), pure grade.

Ionic associate of the cationic complex of polysorbate with barium ions and 12-molybdo-phosphate acid was used as an electrode active substance.

2. 2. Devices used for making and testing of the potentiometric sensor for polysorbate 20 detection

An electrochemical cell (Fig. 2) was used for direct potentiometric studies:



Fig. 2. The electrochemical circle of special cell for direct potentiometry

The galvanic cell consisted of a film potentiometric sensor (with an internal solution 5.0·10⁻⁵ M solution of the test substance and an internal electrode – Ag/AgCl wire in KCl_{sat.}) and silver chloride reference electrode EBL-1M31 with KCl saturated solution. Measurement of EMF is carried out with the ionomer I-130. To determine the pH has used the electrode with brand ESK-10601/4.

2. 3. Method for the synthesis of a plasticized membrane potentiometric sensor sensitive to polysorbate-20

Plasticized polyvinyl chloride membranes were synthesized according to the following procedure: 0.45 g of polyvinyl chloride was dissolved in 4.5 ml of cyclohexanone with weak heating (does not exceed 60 °C) with constant stirring up to complete dissolution. Separately, we prepared a solution of a sample of 0.01 g or 0.10 g of the ionic associate in 1.1 ml of a plasticizer solvent. The phthalic acid esters were chosen as a plasticizer solvent via dibutyl phthalate (DBF) or dioctyl phthalate (DOF). The solutions were mixed and transferred to Petri dishes with a diameter of 50 mm in the form of a transparent homogeneous liquid mixture. A transparent elastic film of a plasticized PVC membrane was obtained from the mixture after complete evaporation of cyclohexanone in 2–3 days.

2. 4. Determination of optimal conditions for the functioning of the membrane of a potentiometric sensor sensitive to polysorbate-20

The membranes were soaked in a solution of polyoxyethylene sorbitan monolaurate with a concentration of 5.0·10⁻⁵ mol/l before starting measurements for the correct operation of a potentiometric sensor. The electrode function of a potentiometric sensor depends on the properties of the ionic associate and on the nature of the plasticizer solvent for the membrane. The characteristics of potentiometric sensors sensitive to the cationic polysorbate - Ba²⁺ particle were studied on various model solutions. A series of standard solutions PS-20 with concentrations from 1.0·10⁻⁶ to 5.0·10⁻³ mol/l was used to build the calibration graphs inasmuch the critical concentration of micelle-forming of polysorbate-20 is ~1.5·10⁻³ mol/l. This fact means that micelles and molecules appear in the solution which can influence on the determination results. Barium nitrate with volume 1.0 ml and concentration at 0.1 mol/l was added to 25.0 ml of each solution in the series to obtain a cationic complex.

The electrode characteristics of the developed sensors (minimum detectable concentration, linearity interval, and sensitivity S) were investigated depending on the various factors to determine the optimal conditions.

3. The results of the development of a potentiometric sensor sensitive to polysorbate20: determination of optimal conditions for the functioning of the membrane

3. 1. Study of the influence of various factors on the slope of the electrode membrane function of a potentiometric sensor sensitive to polysorbate 20

Fig. 3, 4 shows the study results of the effect of pH of the test solution, the nature of the membrane solvent and the quantitative content of the ionic associate in the membrane on the

amount of slope (steepness) of the electrode function of the potentiometric sensor sensitive to polysorbate-20.

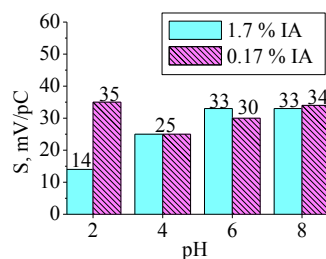


Fig. 3. Dependence of the slope of the electrode function from various factors (plasticizer solvent – diethyl phthalate)

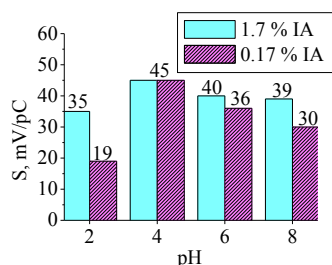


Fig. 4. Dependence of the slope of the electrode function from various factors (plasticizer solvent – dibutyl phthalate)

In the study of the influence of pH of solutions of the standard polysorbate-20 series, it can be seen that the numerical values of the inclination of the electrode function close to the theoretical one are observed at pH=6–8. The nature of the plasticizer solvent and the quantitative content of the ionic associate in the membrane do not have a significant effect on the inclination value of the electrode function of the developed potentiometric sensor sensitive to polysorbate-20

3. 2. The study of the dependence of the minimum determined concentration of polysorbate 20 on various factors

Fig. 5, 6 show the results of a study of the effect of the nature of the solvent, the content of the ionic associate in the membrane and the pH of the test solution on the minimum detectable concentration for the developed potentiometric sensors for polyoxyethylene sorbitan monolaurate.

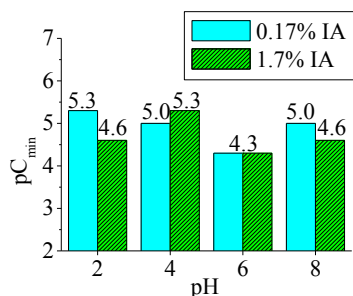


Fig. 5. The influence of various factors on the minimum detectable concentration of PS-20 (plasticizer solvent – diethyl phthalate)

When investigating the effect of the nature of the solvent-plasticizer on the value of the minimum determined concentration, it was found that the lowest concentrations (the highest values of pC) were detected using dibutyl phthalate as a solvent. The acidity of the investigated solution and the quantitative content of the ionic associate in the membrane do not significantly affect this parameter.

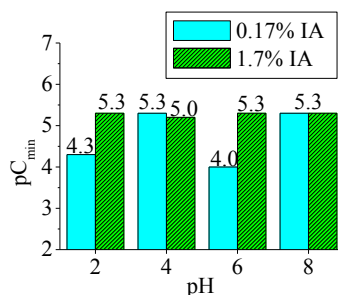


Fig. 6. The influence of various factors on the minimum detectable concentration of PS-20 (solvent – dibutyl phthalate)

3. 3. Investigation of the influence of various factors on the lower limit of the determination of potentiometric sensors sensitive to polysorbate-20

Fig. 7, 8 show the results of a study of the effect of the pH of the test solution, the nature of the solvent and the content of the ionic associate in the membrane on the lower limit of linearity for the developed potentiometric sensors for polyoxyethylene sorbitan monolaurate.

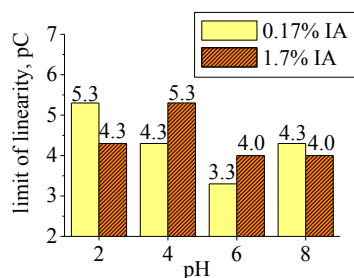


Fig. 7. The influence of various factors on the lower limit of the linearity of the E – pC dependence (solvent – dioctyl phthalate)

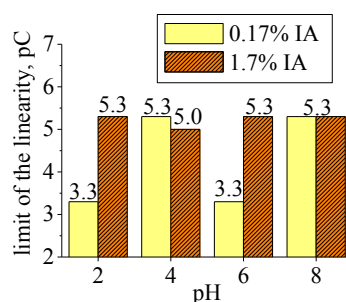


Fig. 8. The influence of various factors on the lower limit of the linearity of the E – pC dependence (solvent – dibutyl phthalate)

The study of the influence of various factors on the lower limit of the linearity of the electrode function showed that the maximum values of pC are observed with the use of a diluent-plasticizer of dibutyl phthalate, the quantitative content of the ionic associate in the membrane and the pH of the solution investigated do not significantly affect this parameter.

4. Discussion of development results and testing of a potentiometric sensor sensitive to polysorbate-20

It was found during the study of the influence of various factors on the steepness of the electrode function of the membrane of the obtained sensor that the slope value is 27–33 mV/pC for

both solvents at a pH of 6 (for DOF) and 8 which corresponds to the theoretical Nernst's value for a double charged cation.

It can be seen from the obtained experimental data, that the best parameters (maximum range of operating concentrations of potentiometric sensors, the lowest detectable concentration ($\sim 5 \times 10^{-6}$ mol/l) and the linearity of the calibration graph up to the concentration of 5.0×10^{-6} M) are observed for membranes with an inclination of the electrode function characteristic of a doubly charged cation under pH=6 and 8 and using of dibutyl phthalate as a membrane solvent and the content of the ionic associate is 0.17 % (0.01 g).

Accordingly, the optimal operating conditions of the potentiometric sensor for polysorbate-20 (linearity interval of the dependence $E=f(PC)$ from $5.0 \cdot 10^{-6}$ to $5.0 \cdot 10^{-3}$ mol/l with the slope of the electrode function $S \approx 30$ mV/pC equal to the Nernst's value for doubly charged cations) are:

- $m_{IA} = 0.01$ g (0.17 %);
- a solvent is dibutyl phthalate;
- pH=8.

In Fig. 9 shows the dependence of the electrode potential of the developed potentiometric sensor for polysorbate-20 on the concentration of the test solution.

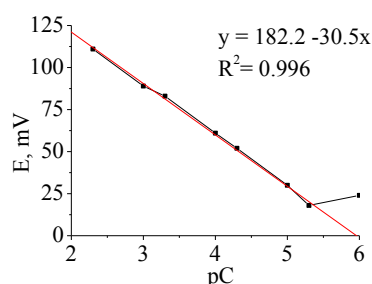


Fig. 9. The dependence of the electrode potential of the developed sensor on the logarithm of concentration ($m_{IA} = 0.01$ g, solvent – DBF, pH=8)

It was experimentally established that the response time of the sensor is 30–50 s depending on the concentration of the test solution, the sensor's lifetime is ~ 50 days at stored dry and soaked for 10–15 minutes in a PS-Ba²⁺ solution with concentration $5.0 \cdot 10^{-5}$ mol/l.

5. Conclusions

The ion associate of the composition $(PS-Ba)_3(PMo_{12}O_{40})_2$ with Keggin structure has been synthesized. It was used as electrode active substances for the construction of polyvinyl chloride membranes of potentiometric sensors sensitive to polysorbate-20. The influence of various factors (the nature of the membrane solvent, the amount of associate in the membrane and the pH of a series of standard solutions) on the electrode characteristics (minimum detectable concentration, linearity interval, and sensitivity S) of the developed sensors was investigated. The optimum composition of the membrane of a potentiometric sensor and the conditions of its operation were selected (the content of the ion associate in the membrane is 0.17 %, a solvent is dibutyl phthalate and pH=8). The developed sensor can be used to determine the quantitative content of polysorbate 20 in various types of industrial products.

References

- [1] Zhilong, L. (2015). Pat. No. CN104666236A. Moisturizing skincare mask. PRC IPC A61K 8/99, A61K 8/97, A61Q 19/00, A61Q 19/08. No. CN201510075282.6A; declared: 13.02.2015; published: 03.06.2015, 13.
- [2] Felipe, J., Lyndon, G., Susan, G., Senad, I. (2015). Pat. WO/2015/164433 USA. Acne solution. IPC A61K 31/05, A61K 36/487, A61K 36/60, A61P 17/10, A61K 47/00. No. 61/982,229 US; declared: 21.04.2014; published: 29.10.2015.
- [3] Ledencova, M. A., Necvetaev, V. V., Smirnova, I. V., Necvetaev, V. V. (2012). Pat. 2491913 RU. Kosmeticheskaya kompoziciya dlya izgotovleniya sredstv po uhotu za volosami. IPC A61K 8/44, A61K 8/64, A61K 8/60, A61K 8/67, A61K 8/98, A61Q 5/12, A61Q 7/00. No. 2012104789/15; declared: 03.02.2012; published: 10.09.2013, Bul. No. 25, 8.

- [4] Belous, E. Yu., Maltabar, S. A., Galimova, A. Z. (2009). Pat. 2414210 RU. Sredstvo dlya udaleniya tabachnyh smol i kompozicii na ego osnove. IPC A61K 8/97, A61K 8/18, A61Q 11/02. No. 2009148450/15; declared: 28.01.2009; published: 20.03.2011, Bul. No. 8, 22.
- [5] State Pharmacopoeia of the Republic of Belarus (2007). Minsk, 471.
- [6] Fekete, S., Ganzler, K., Fekete, J. (2010). Simultaneous determination of polysorbate 20 and unbound polyethylene-glycol in protein solutions using new core-shell reversed phase column and condensation nucleation light scattering detection. *Journal of Chromatography A*, 1217 (40), 6258–6266. doi: <https://doi.org/10.1016/j.chroma.2010.08.028>
- [7] Sparreboom, A., Zhao, M., Brahmer, J. R., Verweij, J., Baker, S. D. (2002). Determination of the docetaxel vehicle, polysorbate 80, in patient samples by liquid chromatography–tandem mass spectrometry. *Journal of Chromatography B*, 773 (2), 183–190. doi: [https://doi.org/10.1016/s1570-0232\(02\)00167-8](https://doi.org/10.1016/s1570-0232(02)00167-8)
- [8] Prasad Durga, V., Rangareddy, V., Aparna, P., Sudner babu, K., Prasad, N. N. (2015). HPLC-ELSD Determination of Sodium Lauryl Sulphate and Polysorbate in Nebivolol Drug Product and Different Formulation Products. *International Journal of Pharmaceutical Sciences and Research*, 6 (8), 3612–3616.
- [9] Őszi, Z., Pethő, G. (1998). Quantitative determination of polysorbate 20 in nasal pharmaceutical preparations by high-performance liquid chromatography. *Journal of Pharmaceutical and Biomedical Analysis*, 18 (4-5), 715–720. doi: [https://doi.org/10.1016/s0731-7085\(98\)00265-9](https://doi.org/10.1016/s0731-7085(98)00265-9)
- [10] Nair, L. M., Stephens, N. V., Vincent, S., Raghavan, N., Sand, P. J. (2003). Determination of polysorbate 80 in parenteral formulations by high-performance liquid chromatography and evaporative light scattering detection. *Journal of Chromatography A*, 1012 (1), 81–86. doi: [https://doi.org/10.1016/s0021-9673\(03\)01105-1](https://doi.org/10.1016/s0021-9673(03)01105-1)
- [11] Tkach, V. I. (1999). Geteropolianiony struktury Keggina kak analiticheskie reagenty na azotsoderzhashchie organicheskie veshchestva. Dnipropetrovsk: National University, 321.
- [12] Kumaniova, M. O., Tkach, V. I. (2011). Analysis of the salts of polyhexamethyleneguanidine in industrial objects by electrochemical methods. *Methods and objects of chemical analysis*, 6 (3), 169–181.
- [13] Volnians'ka, O. V., Labyak, O. V., Tkach, V. I. (2015). Potentiometric determination of thiabendazole in food products. *Issues of Chemistry and Chemical Technology*, 4, 4–8.
- [14] Volnyanska, O. V., Labyak, O. V., Blazheyevskiy, M. Ye., Brizitskiy, O. A., Tkach, V. I. (2016). Amperometric and spectrophotometric determination of food additive thiabendazole (E-233) in Bananas. *International Journal of Advances in Pharmacy, Biology and Chemistry*, 5 (3), 271–281.
- [15] Lutsenko, N., Mironyak, M., Panchenko, J., Tkach, V. (2016). Ionometric Determination of Tannins in Industrial Production. *Chemistry & Chemical Technology*, 10 (1), 73–80. doi: <https://doi.org/10.23939/chcht10.01.073>
- [16] Lutsenko, N. V., Mironyak, M. A., Labyak, O. V., Volnyanska, O. V., Tkach, V. I. (2016). Determination of the total content of diterpene glycosides in *Stevia rebaudiana* plant by the method of direct potentiometry. *Der Chemica Sinica*, 7 (1), 9–19.
- [17] Mironyak, M. A., Volnyanskaya, E. V., Tkach, V. I. (2017). Ionnye asociaty guanidinovyh polielektrolitov s geteropolianionami. Saarbrücken: LAP LAMBERT Academic Publishing, 141.
- [18] Lutsenko, N. V., Tkach, V. I., Mironyak, M. A., Shtemenko, O. V. (2016). Pat. No. 116399 UA. Sposib kilkisnoho vyznachennia hlitsyryzynu v kharchovykh produktakh ta kosmetychnykh ta farmatsevtichnykh zasobakh. IPC G01N 27/40. No. u2016108788; declared: 15.08.2016; published: 25.05.2017, Bul. No. 10, 4.
- [19] Volnyanskaya, O., Mironyak, M., Nikolenko, M. (2018). Potenciometrichni sensori dlya viznachennya nitrogenvmisnih rechovin. Saarbrücken: LAP LAMBERT Academic Publishing, 109.
- [20] Volnyanska, O. V., Labyak, O. V., Blazheyevskiy, M. Y., Brizitskiy, O. A., et. al. (2018). Electrochemical Method For Determination Of Cyclamate Using 12-Molybdophosphoric Acid. *Methods and Objects of Chemical Analysis*, 13 (1), 29–34. doi: <https://doi.org/10.17721/moca.2018.29-34>

Received date 24.06.2019

Accepted date 12.07.2019

Published date 31.07.2019

© The Author(s) 2019

This is an open access article under the CC BY license
(<http://creativecommons.org/licenses/by/4.0>).