

RESEARCH ARTICLE

DEVELOPMENT, VALIDATION & STRESS DEGRADATION STUDIES OF TRIPROLIDINE BY REVERSE PHASE-HIGH PERFORMANCE LIQUID CHROMATOGRAPHY (RP-HPLC)

PVSR Mohana Rao¹, Tata Santosh², Dr. K Raghu Babu^{1*}¹Andhra University College of Engineering, Andhra University, Andhra Pradesh, India.²Corpuscle Research Solutions, Andhra Pradesh, India.*Date Received: 30th January 2016; Date Accepted: 11th February 2016 Date published: 12th February 2016*Email: draggualways@yahoo.co.in

Abstract: Objective: To develop a simple, selective and precise and rapid reverse phase high performance liquid chromatography method for the development and validation, stress degradation studies of Triprolidine in bulk and Pharmaceutical dosage forms. **Methods:** The chromatographic separations was performed by Agilent Polaris C₁₈ column (150 X 4.6 mm id, ODS 2.5 μ m) using methanol: 0.1% ortho-phosphoric acid in water (65:35) as mobile phase at flow rate of 0.1 mL/min with injection volume 20 μ L and the detection was carried out using UV detector at 232nm. The method was validated as per ICH guidelines. **Results:** The retention time for Triprolidine was found to be 1.88 min respectively. The linear regression analysis data for the calibration plots showed good linear relationship in the concentration range of 1.01-10.05 μ g/mL. The correlation coefficient and percent recovery for Triprolidine were found to be 0.9989 and 100.66 respectively. The influence of Acid, Alkaline, Oxidative stress, Photolytic stress condition on Triprolidine was studied. Results indicated completed degradation in Alkaline medium. **Conclusion:** The developed method was successfully validated in accordance to ICH guidelines. This

method is simple, selective, linear and precise accurate and sensitive and can be used for routine analysis of bulk samples.

Key words: Triprolidine; HPLC, Stress Degradation.

Introduction

Triprolidine is chemically 2-[(1E)-1-(4-methylphenyl)-3-(pyrrolidin-1-yl)prop-1-en-1-yl] pyridine (Fig.1), Anti-allergic, Histamine H1 Antagonist that block the action of endogenous histamine, which subsequently leads to temporary relief of negative symptoms brought on by histamine. It is used for the treatment of seasonal or perennial allergic rhinitis or non allergic rhinitis, conjunctivitis and mild urticaria and angioedema[1]. The most common side effects are sedation, dizziness, incoordination, gastrointestinal disturbances, nausea, vomiting and diarrhea. It may also produce blurred vision, dryness of mouth, tight of chest, blood disorders including agranulocytosis and haemolytic anaemia[2]. Literature survey revealed that few analytical methods have been reported; determination of Triproline in plasma using Thin layer chromatography[3]; simultaneous determination of Triprolidine with other anti-histamines [3][4][5]; other agents[6][7]; Few methods had been developed for determination of Triprolidine by HPLC[8] and Spectrophotometric method[9]; Spectrophotometric and High Performance Liquid Chromatographic [10]. Determination of Triprolidine and its metabolite in biological samples using liquid chromatography-mass spectrometry[11]. Capillary Zone Electrophoresis Method for Quality Control Analysis of Triprolidine with other drugs[12]; Degradation studies of Triprolidine and Stability indicating UPLC method[13]; New plastic membrane and carbon paste ion selective electrodes for determination of triprolidine[14]. Triprolidine is usually administered in combination with dextromethorphan and/or phenylpropanolamine and also with paracetamol. [15]

Reported HPLC methods have lesser throughput and are occasionally lacking the stress behaviour studies. Hence there is no simple, cost effective individual method have been reported. Therefore, the present work involves the development of a rapid RP-HPLC method for estimation of Triprolidine in bulk and tablet dosage form. Validation as per USFDA & ICH guidelines [16], [17] is done along with stress degradation study. The aim of the present study is to develop a simple, precise and accurate reversed-phase HPLC method for the development and validation of Triprolidine in bulk drug samples and in pharmaceutical dosage form.

2. EXPERIMENTAL

2.1 Reagents and Chemicals

Methanol (HPLC grade, Merck Ltd), Milli-Q water, Troprolidine (Reference standard purchased from Sigma Aldrich, USA), 0.1% Ortho-Phosphoric acid (GR Grade, SD Fine Chem Ltd). All other chemicals are of the highest grade commercially available unless otherwise specified.

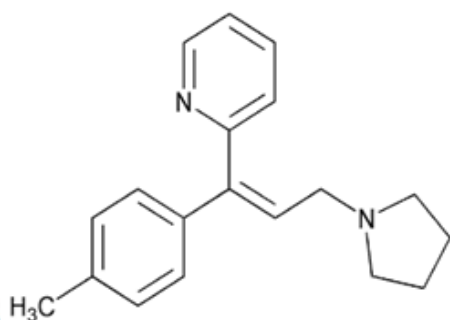


Fig. 1: Structure of Troprolidine

2.2 Instrumentation

The chromatographic system consisted of a Shimadzu Class VP Binary pump LC-10ATvp, SIL-10ADvp Auto sampler, CTO-10Avp Column Temperature Oven, SPD-10Avp UV-Visible detector. All the components of the system are controlled using SCL-10Avp System Controller. Data acquisition was done using LC solutions software.

2.3 Chromatographic Conditions

The mobile phase consisted of 65:35 % (v/v) of Methanol & 0.1% Ortho-phosphoric acid operated on isocratic mode. The flow rate is 1.0 ml/min. Chromatographic determination of Troprolidine was performed on Agilent Polaris C₁₈ column (150 X 4.6mm id, ODS 2.5μm). The effluent was monitored by UV detector at 232. The injection volume is 20μL.

2.4 Preparation of Standard solutions

Stock solution of Troprolidine was prepared by dissolving 10 mg drug in diluent solution (50:50 % v/v Methanol & Milli-Q water), Sonicated and then make the volume upto 100mL. The concentration of stock solution was found to be 100 μg/mL. The working standard solutions of Troprolidine was prepared by taking suitable aliquots of drug solution from the working stock solution and the volume was made upto 10 mL with mobile phase to get concentrations of 1.01 to 10.05. These solutions were filtered through 0.45μ membrane filter before injection and 20μL of solution was injected to the chromatographic system.

2.4.1 Preparation of sample solution

Ten tablets of Troprolidine were taken individually and

their weight is taken. The average weight of each tablet is calculated. Tablet powder equivalent to 1 tablet powder is then weighed accurately and transferred into a 100mL volumetric flask. 70mL of diluent was then added and sonicated to dissolve it completely and made volume up to the mark with the diluent. The solution is mixed well and filtered through 0.45μm filter. 1mL of the solution is then transferred into a 10mL volumetric flask and diluted up to the mark with diluent. The final solution was mixed well. This mixture is then carefully filtered using 0.45μm membrane filter. The filtrate is then taken and suitably diluted and injected for analysis. The assay content was evaluated using the regression equation of linear calibration curve.

3. RESULTS AND DISCUSSION

HPLC separation of Troprolidine was carried out on a Agilent Polaris C₁₈ column by an isocratic elution with of Methanol & 0.1% Ortho-phosphoric acid (65:35 % v/v). The flow rate was constant at 0.8mL/min and the column temperature was at ambient temperature. The UV wavelength was set at 232 nm. No interference from diluents, impurities or excipients present in the pharmaceutical formulation was observed at this detection wavelength. Before each run LC column was equilibrated with the mobile phase for about 15 min. A sharp, symmetrical peak was obtained for Troprolidine when analyzed under these conditions. This retention time enable rapid determination of the drug, which is important for routine quality control analysis. A typical chromatogram showing the separation of the drug is given in Fig-2.

System suitability test was established from six replicate injections of a solution containing Troprolidine 5 μg/mL. The percent relative standard deviation (RSD) of the peak area was calculated. The peak tailing for drug was measured. A useful and practical measurement of peak shape, the peak tailing and theoretical plate count was determined. The proposed method met these requirements within the United States Pharmacopoeia (USP) accepted limits (Tailing factor < 1.5, Theoretical plates > 2000). The stability of Troprolidine in solution was investigated in the method development phase. six solutions containing 10 μg/mL of Troprolidine were tested. The solutions were stable during the investigated time and the RSD was < 1.0% for retention time (min), peak area and height. The solutions were shown to be stable with no significant change in Troprolidine concentration over this period Table.1 .

Method Validation

Linearity

Appropriate amounts of Troprolidine stock solutions were diluted with mobile phase to give concentration of

1.02, 2, 4, 6, 8 and 10.05 µg/ml. Each solution was injected calibration plot was prepared. Linearity was evaluated by linear least-squares regression analysis. Good linearity was observed over the concentration range evaluated (1-

10 µg/ml) as shown in the linearity curve in Figure 3. The correlation coefficient was found 0.999. The results are tabulated in Table 2

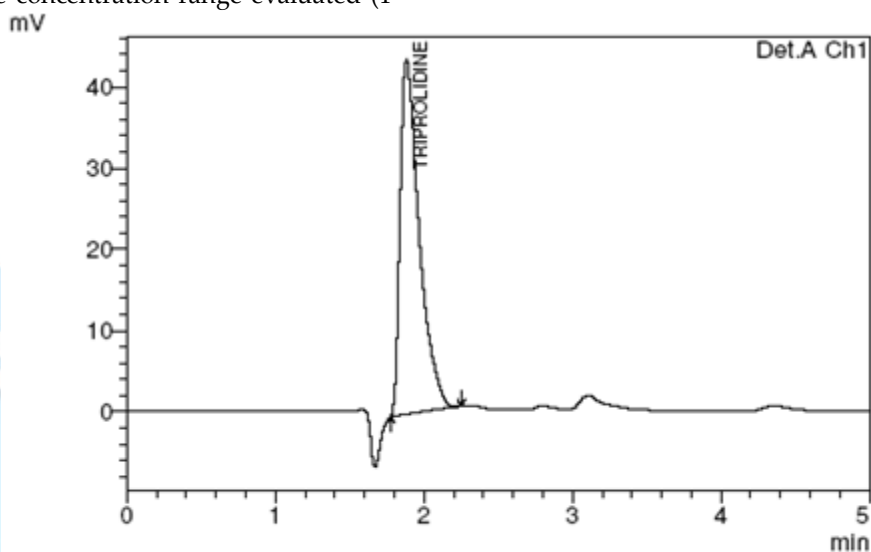


Fig. 2 : Typical Chromatogram of Triprolidine

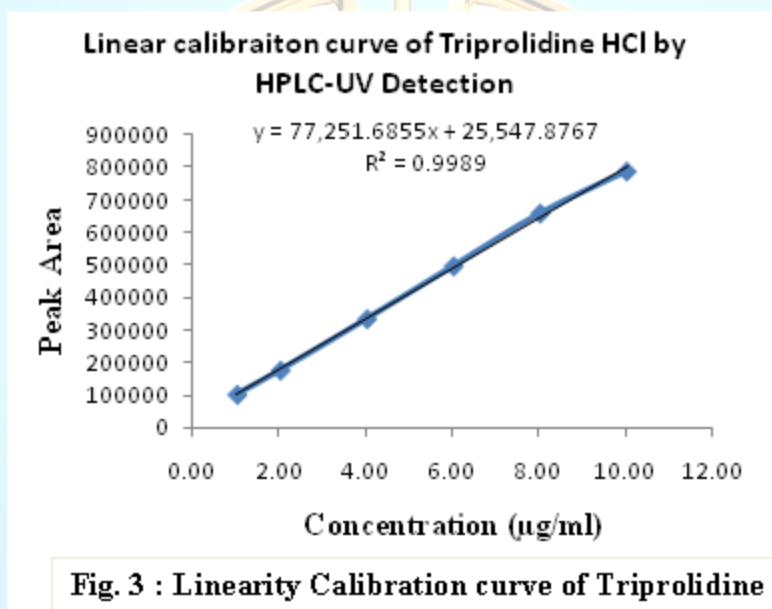


Fig. 3 : Linearity Calibration curve of Triprolidine

Table 1. System Suitability test for Triprolidine

S.No	Retention Time	Peak Area	Theoretical Plates	Tailing factor
1	1.88	389705	5993	1.73
2	1.88	383481	5949	1.74
3	1.88	385619	6092	1.74
4	1.89	381912	6099	1.74
5	1.88	390329	5918	1.70
6	1.88	399277	6186	1.74
Mean	1.88	388387	6039.50	1.73
Std.Dev	0.00	6288.99	102.83	0.02
%CV	0.22	1.62	1.70	0.93

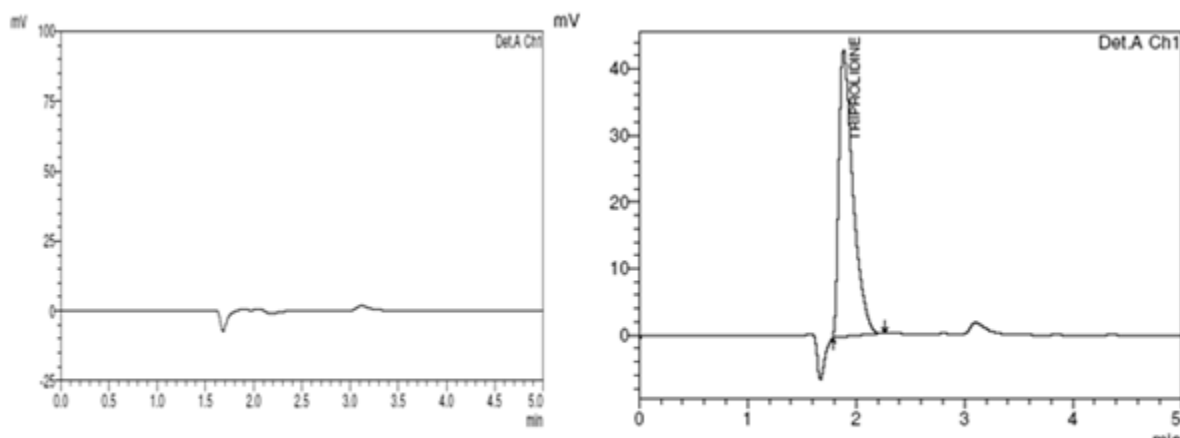


Fig. 4 : Comparison of Blank Chromatogram to that of sample containing Triprolidine

Table 2. Statistical data of Linearity for Triprolidine by RP-HPLC method

Parameter	Value
Absorption maximum (nm)	232
Linearity range (µg/mL)	1.01-10.05
Regression equation	$Y = 77251x - 25547$
Correlation coefficient	$R^2 = 0.9989$
Slope	77251
Intercept	25547

Table 3 : Precision of the proposed method

Conc. (µg/mL)	Intra-day Precision		Inter-day Precision	
	Mean Area	% RSD	Mean Area	% RSD
2.51	220960	1.06	220006	1.41
5.03	418350	0.67	417584	0.80
7.54	613135	0.80	610544	1.47

Table 4: Accuracy of the proposed method

Theoretical Conc. (µg/mL)	Measured Conc. (µg/mL)	% Recovery	% RSD
2.51	2.51 ± 0.03	100.66	1.20
5.03	5.09 ± 0.04	101.12	0.71
7.54	7.61 ± 0.06	100.96	0.83

Table 5. Sensitivity of Triprolidine by HPLC

LOQ		
S.No	Retention Time	Peak Area
1	1.88	38678
2	1.89	37459
3	1.88	38187
Mean	1.88	38108
Std.Dev	0.01	613.33
%CV	0.31	1.61

LOD		
S.No	Retention Time	Peak Area
1	1.88	18678
2	1.89	18459
3	1.88	19187
Mean	1.88	18774
Std.Dev	0.01	373.50
%CV	0.31	1.99

Table 6. Robustness Data

Parameters	Optimized method	Used adopted for robustness	Peak Area	Retention Time	USP plate count	Tailing
Flow rate (ml/min) (± 0.1)	1.0 mL	0.9mL/min	394449	1.85	3021	2.0
		1.0 mL/min	380337	1.88	6046	1.74
		1.1 mL/min	486060	2.26	3527	1.8
Mobile Phase ($\pm 5\%$ Organic Composition)	65:35 (%)	70:30	527487	1.78	1791	1.9
		65:35	382620	1.88	6036	1.73
		60:40	378941	2.03	3183	2.0

Table 7: Stress Degradation study data for Triprolidine

Degradation Condition	Peak Area	Peak Area (%)
Acidic hydrolysis (0.1% HCl)	417204	100.3
Oxidation (5% H ₂ O ₂)	417038	100.3
Photolytic degradation (UV light)	422803	101.7
Control sample	415627	-

Precision

The precision of the method was investigated with respect to repeatability and intermediate precision. The repeatability (intra-day precision) of the method was evaluated by assaying three replicate injections of the Triprolidine at 100% of test concentration (5 μ g/ml) on the same day. The %RSD of the retention time (min) and peak area were calculated. Intermediate precision (inter-day precision) was demonstrated by evaluating the relative peak area percent data the LC system at three different concentration levels that cover the assay method range (2-10 μ g/ml). The %RSD of the system was calculated from the individual relative percent peak area mean values of the test concentration (Table 3). The intra-day ($n=3$) and inter-day ($n=3$) %RSD are given in table. All the data are within the acceptance criteria of 2%.

Accuracy

Accuracy of the method was evaluated by fortifying a Triprolidine sample solution (with respect to the target assay concentration) with three known concentrations of reference standard (2, 5 and 7 μ g/ml). Percent recoveries were calculated from differences between the peak areas obtained for fortified and unfortified solutions. Good recoveries were obtained within the acceptance criteria (98.0-102.0%) as shown in Table 4.

LOD & LOQ

Limits of detection (LOD) and quantification (LOQ) were estimated from both linearity calibration curve method and signal to noise ratio method. The detection limit was defined as the lowest concentration level resulting in a peak area of three times the baseline noise. The quantification limit was defined as the lowest concentration level that provided a peak area with signal to noise ratio higher than 5, with precision (%CV) and accuracy with (\pm) 20%.

Limit of Detection (LOD) and Limit of Quantification (LOQ) were calculated based on calibration curves. They were expressed as $LOD = (3.3 \times \sigma)/S$; $LOQ = (10 \times \sigma)/S$ (where σ is the standard deviation of the y-intercepts of the regression line and m is the mean of the slope of the calibration curve). The method is found to be sensitive which can be determined from the data obtained from the (Table 5).

Specificity

Specificity of the method was determined by comparing the Blank sample with that of the sample containing Triprolidine. A less than 20% interference of the peak area at the retention time of the drug in the blank sample is

taken as acceptance criteria for the analyte. Sample Specificity is also observed in the degradation study of the drug. None of the degraded products must interfere with the quantification of the drug. Specificity of the method was observed by injecting the blank and working standard solutions of Triprolidine. The specificity was determined by comparison of the blank chromatogram with that of the Standard chromatogram (Fig. 4).

Robustness

Robustness of the method was evaluated by the analysis of Triprolidine under different experimental conditions such as changes in the organic composition of the mobile phase and flow rate. The percentage of methanol in the mobile phase was varied $\pm 10\%$, the flow rate was varied ± 0.1 ml/min. Their effects on the USP plate count, USP tailing at 10%, recovery and repeatability were studied. Deliberate variation of the method conditions had no significant effect on assay data or on chromatographic performance, indicating the robustness of method and its suitability for routine use and transfer to other laboratories. The results from robustness testing are presented in Table 6.

Stress Degradation Studies

For Stress Degradation Analysis, 1 mL aliquots (in duplicate) of samples containing MQC level concentration are treated separately with 100 μ L of 0.1N HCl (Acid stress), 0.1N NaOH (Alkaline stress), 5% v/v Hydrogen Peroxide (Oxidative Stress), for 24 Hrs. Samples for Photolytic stress are placed in a transparent glass vial & placed in a UV chamber for 24 Hrs. Samples are then injected for analysis. The results of analysis are then compared with similarly prepared fresh samples.

The stress studies involving acid, light (UV) and oxidation revealed that Triprolidine was not fully degraded. However in alkaline conditions (0.1N NaOH), the drug was instable and the degradation peak eluted earlier accompanied with a drastic peak distortion and increased tailing. Except for alkaline conditions, the drug content was within 95 –105 % for all stress conditions indicating the stability and specificity of the analytical method to differentiate the degradation peaks. (Table-7)

CONCLUSION

A rapid, accurate and precise isocratic RP-HPLC method has been developed. The developed was found to be simple and have short run time which makes them method rapid. The chromatographic run time of 10 min allow analysis of lot of samples in a short period of time. Therefore, the method is suitable for analysis of large samples during routine analysis of formulations and raw materials. Nevertheless, the results of the study indicate that the

developed HPLC method is simple, precise, accurate and less time consuming.

ACKNOWLEDGEMENT

The authors are thankful to Mr. Santosh Tata, CorpuScle Research Solutions, Visakhapatnam, India, for providing the necessary facilities to carry out this work.

Conflict of Interest

Authors do not have any conflict of interest in this research work.

REFERENCES

1. Drug Profile, "Triprolidine" <http://www.mims.com/Troprolidine>
2. Reynolds, J.E.F. 1982. Promethazine and other anti-histamines. In: Martindale: The Extra Pharmacopoeia, 28th Edition, pp.1294. The Pharmaceutical press, London.
3. R.L. Deangelis, M.F. Kearney and R. M. Welch. (1997). Determination of triprolidine in human plasma by quantitative TLC. Journal of Pharmaceutical Sciences.66 (6), 841-843.
4. Arvind Gupta, Rajesh Kumar Nema, Atul sahu. (2009). Simultaneous estimation of Phenylpropanolamine hydrochloride and Triprolidine hydrochloride in pharmaceutical preparations by RP-HPLC method. The Pharma Research.1;67-71.
5. Hetice Caglar, Ebru Buyuktuncel.(2014). HPLC method development and validation: Simultaneous determination of active ingredients in cough and cold Pharmacueticala. International journal of pharmacy and pharmaceutical sciences. 6(10), 421-428.
6. Yasser EL-Shabrawy, Alaa El-Gindy, Maisra Al-Shabraw Shoeib and Yassmin El-Gindy. (2014). An HPLC method for Determination of 15 Pharmaceutical compounds in Anti-cold Products. Standard Research Journal of Pharmacy and Pharmacology. 1(4), 86-94.
7. Alaa El-Gindya, Khalid Abdel-Salam Attiab, Mohammad Wafaa N assarb, Hamed Abu Aeadab and Maisra Al-Shabrawi Shoeibc. (2013). HPLC method for determination of Paracetamol, Psudoephedrine, Triprolidine, Methylparaben, Propylparaben, Sodium Benzoate and other related substances in Pharmaceutical syrup. Journal of liquid cheomatography & related technologies. 36(9), 1251-1263.
8. Basel M. Saida, Shrhabeel A.Alabjaw, Fawaz Deabas, Munib M. Saket, Rami Shareiah and Eyad S. M.Abu Nameh. (2014). Liquid chromatographic Method for the Determination of Triprolidine. Journal of chemical and Pharmaceutical Research, 6(8), 327-332.
9. Amina Mumtaz, Asrar A.Kazi, Tehseen Aman, M. Usman Sabri and Fauzia Noureen. (2005). Dtermination of Tropolidine-Hcl by Spectrophoto-

- metric method in pure and pharmaceutical preparations using Dichloronitrobenzene as a new chemogenic reagent. *Proc.Pakistan Acad.Sci.* 42(4), 253-259.
10. Madhuri Hinge, K.R.Patel and R.J.Mahinda. (2015). Spectrophotometric and High performance liquid chromatographic determination (HPLC) of Triprolidine and Pseudoephedrine hydrochloride in Tablet dosage form. *Pharm Method.* 15(6), 87-93.
 11. Hansen EBJr, Getek TA, Korfmacher WA. (1989). Application of HPLC-Thermospray ionization mass spectrometry for the analysis of Triprolidine and its metabolite hydromethytriprolidine in biological samples. *J Anal Toxicol.* 13(3), 185-187.
 12. Sonia Di Berardino, Renata Jasionowska. (2014). Rapid and sensitive CZE (capillary zone electrophoresis) method for Quality Control analysis of Pharmaceuticals containing Pseudoephedrine, Triprolidine and Paracetamol. *American Journal of Analytical Chemistry.* 5:613-619.
 13. Mahesh Kumar Moneab, K.B. Chandrasekh & Samir Vyasa. (2011). Degradation studies of Triprolidine: Isolation, Characterization of oxidative Degradation products and Development of a validated stability indicating method UPLC method. *Journal of Chromatography & Related Technologies.* 34(8), 652-669.
 14. Zayed, S.I. 2004. New plastic membrane and carbon paste ion selective electrodes for the determination of Triprolidine. *Anal. Sci.* 20:1043-1048.
 15. C E Bye, J Cooper, D W Empey, A S Fowle, D T Hughes, E Letley, and J O'Grady (1980) Effects of pseudoephedrine and triprolidine, alone and in combination, on symptoms of the common cold. *Br Med J.* 1980 Jul 19; 281(6234): 189-190.
 16. Guidance for Industry: Analytical Procedure and methods Validation: Chemistry, Manufacturing and Controls Documentation; Draft Guidance. Rockville, MD. UD FDA. 2000,
 17. International Conference on Harmonization, "Q2A: Text on Validation of Analytical Procedures," Federal Register, 60(40), 1995, 11260-11262.

