

**How to Cite:**

Gulati, M. S., Kumar, M. S., & Arora, J. (2021). Stereolithography in implant placement: A review. *International Journal of Health Sciences*, 5(S2), 23–27.  
<https://doi.org/10.53730/ijhs.v5nS2.5344>

# Stereolithography in implant placement: A review

**Manmeet Singh Gulati**

Professor And Head Of Department, Desh Bhagat Dental College & Hospital, Mandi Gobindgarh, India

**Manmohit Singh Kumar**

Professor Dept. of Prosthodontics and Crown & Bridge Desh Bhagat Dental College And Hospital, Mandi Gobindgarh, India

**Jasleen Arora**

Sr. Lecturer, Dept. of Prosthodontics and Crown & Bridge Desh Bhagat Dental College And Hospital, Mandi Gobindgarh, India


**Abstract**---Stereolithography (SLA), the first form of additive manufacturing, creates 3D objects by selectively solidifying liquid resin via a photopolymerization reaction. Stereolithography has gained popularity due to its ability to fabricate objects with high accuracy and in a wide range of materials. SLA has undergone four generations of major technological innovation since its invention in the 1980s. As a result of these advancements, a diverse range of stereolithography systems with dramatically improved resolution, throughput, and material selection for creating complex 3D objects and devices is now available.

**Keywords**---stereolithography, photopolymerization reaction, implant placement, 3D objects.

**Introduction**

Stereolithography is an additive manufacturing process that works by focusing an ultraviolet (UV) laser on a vat of photopolymer resin in its most common form. Because photopolymers are UV-sensitive, the resin is photochemically solidified and forms a single layer of the desired 3D object. Stereolithography can be used to create prototypes for new products, medical models, and computer hardware, among many other things. While stereolithography is quick and can produce almost any design, it is also costly. Stereolithography (SLA) uses UV lasers as a light source to selectively cure a polymer resin. Digital light processing (DLP) uses

a digital projector as a UV light source to cure a layer of resin. Liquid crystal display (LCD) uses an LCD display module to project specific light patterns.

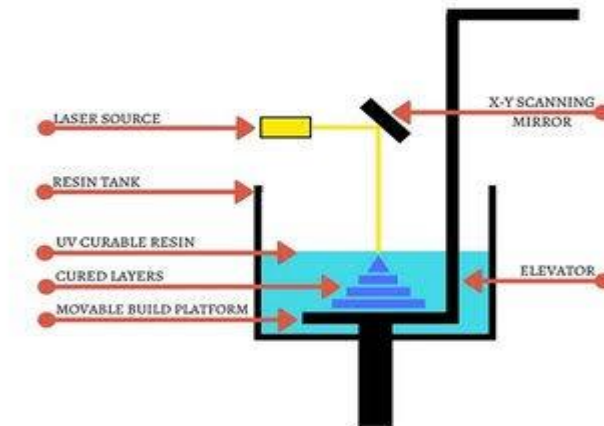

### Techniques of stereolithography

It has three methods:-

- PBF (Powder bed fusion)
- Light Curing
- FDM (Fused deposition modelling)

### Uses

In the field of medicine, such as


- Traumatology
- Cardiology
- Neurosurgery
- Plastic surgery
- Craniomaxillofacial surgery
- In the field of dentistry, its application range
  - Prosthodontics
  - Oral and maxillofacial surgery
  - Oral implantology to orthodontics, endodontics and periodontology

### Uses in prosthodontics

- Production of auricular and nasal prosthesis
- Obturators
- Duplication of existing maxillary/ mandibular prosthesis
- Manufacturing of surgical stents for patients
- Manufacturing of lead shields

## Implantology

The use of computer aided design/computer aided manufacturing (CAD/CAM) technology. The Applications pertain to the three dimensional imaging, 3-D software for treatment planning, fabrication of computer-generated surgical guides using additive RP

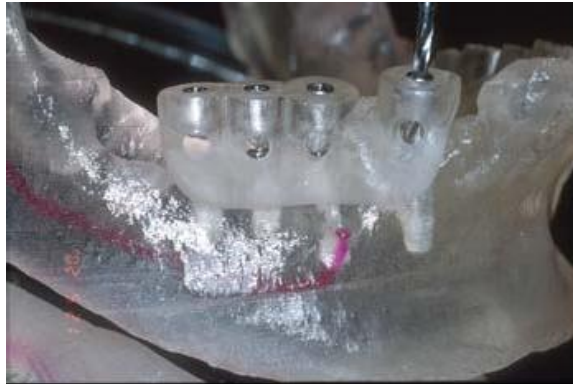

### Advantages

- It has high accuracy.
- It has smooth, high quality surfaces
- High resolution of small details
- It has short turnaround time

### Disadvantages

- It has limited mechanical and thermal strength.
- It requires support structures some designs cannot be printed.


## Technique

### Diagnostic Wax up

Diagnostic study casts are properly articulated on a demo adjustable articulator. After a comprehensive clinical and roentgenographic examination a sound treatment plan is formulated and diagnostic wax up is made up by using irreversible hydrocolloid and a duplicate cast is made with Type IV dental stone. A radiographic template is fabricated on a duplicate study cast.

For a complete dentures, a duplicate of a previously fabricated complete denture can also be used, if the denture contains correct relationships

### Principle of stereolithography

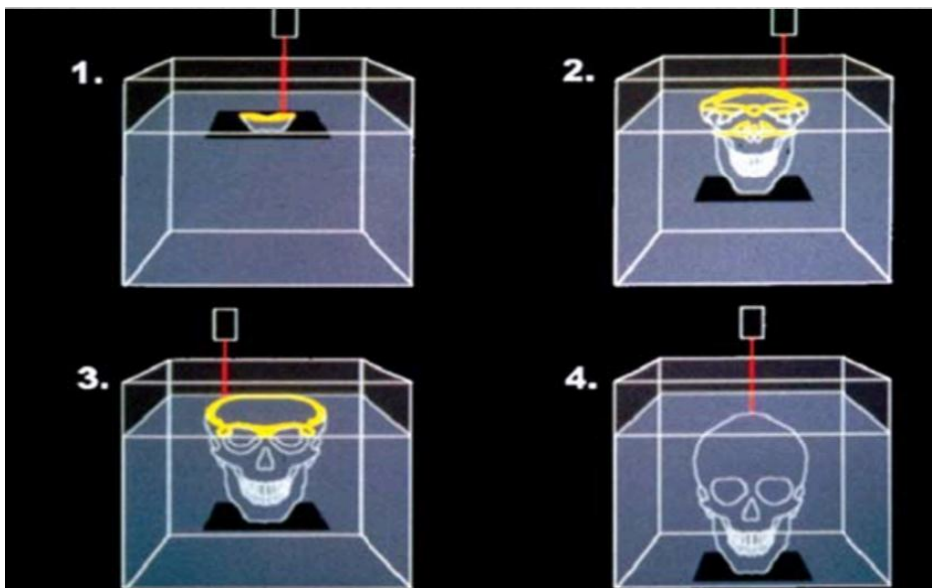

### Conclusion

SLA stereolithography enables the production of parts that adhere to a few simple constraints. Projects requiring prototypes with mechanical and visual properties identical to series parts, on the other hand, must be manufactured using other prototyping techniques. Stereolithographic templates can be used to predictably place surgical and prosthodontic implants. Soft tissue, bone, or remaining teeth can be used to support the templates completely. The cost is higher than with traditional templates, but the benefit may justify the extra expense in more complex, fully edentulous cases

### References

- McGivney GP, Haughton V, Strandt JA, et al: A comparison of computer-assisted tomography and data gathering modalities in prosthodontics. *Int J Oral Maxillofac Implants* 1986;1:55-68

- Fjellstrom CA, Strom C: CT of the edentulous maxilla intended for osseointegrated implants. *J CraniomaxillofacSurg* 1987;15:45-46
- Andersson L, Kuroi M: CT scan prior to installation of osseointegrated implants in the maxilla. *Int J Oral MaxillofacSurg* 1987;16:50-55.
- Petrikowski CG, Pharoah MJ, Schmitt A: Presurgical radiographic assessment for implants. *J Prosthet Dent* 1989;61:59-64
- Schwarz MS, Rothman SL, Chafetz N, et al: Computed tomography in dental implantation surgery. *Dent Clin North Am* 1989;33:555-597.
- Sethi A: Precise site location for implants using CT scans: a technical note. *Int J Oral Maxillofac Implants* 1993;8:433-438
- Todd AD, Gher ME, Quintero G, et al: Interpretation of linear and computed tomograms in the assessment of implant recipient sites. *J Periodontol* 1993;64:1243-1249
- Gillespie JE, Isherwood I: Three-dimensional anatomical images from computed tomographic scans. *Br J Radiol*1986;59:289-292
- B. C. Gross, J. L. Erkal, S. Y. Lockwood, C. Chen, and M. D. Spence, "Evaluation of 3D printing and its potential impact on biotechnology and the chemical sciences," *Analytical Chemistry*, vol. 86, no. 7, pp. 3240–3253, 2014.
- Azari A, Nikzad S. The evolution of rapid prototyping in dentistry: a review. *Rapid Prototyping J* 2009; 15: 216-225.
- G. Oberoi, S. Nitsch, M. Edelmayer, K. Janjić, A. S. Müller, and H. Agis, "3D printing-encompassing the facets of dentistry," *Frontiers in bioengineering and biotechnology*, vol. 6, article 172, 2018
- Prechtel, M. Reymus, D. Edelhoff, R. Hickel, and B. Stawarczyk, "Comparison of various 3D printed and milled PEEK materials: effect of printing direction and artificial aging on Martens parameters," *Dental Materials*, vol. 36, no. 2, pp. 197–209, 2020.
- Sarment DP, Sukovic P, Clinthorne N. Accuracy of implant placement with a stereolithographic surgical guide. *Int J Oral Maxillofac Implants* 2003; 18: 571-577.
- Ruppin J, Popovic A, Strauss M, Spüntrup E, Steiner A, Stoll C. Evaluation of the accuracy of three different computer-aided surgery systems in dental implantology: Optical tracking vs. stereolithographic splint systems. *Clin Oral Implants Res.* 2008;19:709–16.